

**HAPTICS-BASED VIRTUAL REALITY
PERIODONTAL TRAINING SIMULATOR**

BY

CRISTIAN J. LUCIANO

B.S., Computer Science, Universidad Tecnológica Nacional, Argentina, 1994
M.S., Industrial Engineering, University of Illinois at Chicago, 2000

THESIS

Submitted as partial fulfillment of the requirements
for the degree of Master of Science in Computer Science
in the Graduate College of the
University of Illinois at Chicago, 2006

Chicago, Illinois

To my daughters Serena and Florencia
and my wife Paola.

ACKNOWLEDGEMENTS

I would like to thank my advisor Prof. Thomas A. DeFanti and my co-advisor Prof. P. Pat Banerjee for their continuous guidance and support both professionally and personally. I sincerely appreciate them for giving me the great opportunity to learn so much while working at the *Electronic Visualization Laboratory* and the *Industrial Virtual Reality Institute*. I would also like to express my gratitude to Prof. Jason Leigh, who has always been enthusiastic to help and advise me with motivating ideas.

I wish to extend my gratefulness to Dr. Arnold Steinberg and Dr. Jim Drummond for giving me technical feedback and thoughts from dentists' perspective, and to Dr. Bruce Graham, Dean of the UIC College of Dentistry, for showing interest in this project.

This work was funded by the Fulbright-YPF Fellowship and the Link Foundation Fellowship as well as by the UIC Department of Mechanical and Industrial Engineering and the UIC Department of Periodontics.

I want to thank my colleges and good friends Javier Girado and Silvio Rizzi for taking the time to review this thesis and giving me helpful suggestions; and all my close friends from Argentina now living in Chicago, who became more family members than friends after all these years.

I wish to especially thank my wife Paola, and my daughters Serena and Florencia, for their unconditional support and for all the time I could not spend with them as much as I (and they) wanted because of being working on this project.

And last but not least, thanks to my family in Argentina, who I truly miss and love, for their support and encouragement during all these years in the US.

CJL

TABLE OF CONTENTS

<u>CHAPTER</u>	<u>PAGE</u>
1 INTRODUCTION	1
2 BACKGROUND.....	3
2.1 Medical simulators.....	3
2.2 Dental simulators.....	5
2.2.1 Manikin-based dental simulators.....	6
2.2.2 Haptics-based dental simulators.....	9
3 PERIODONTAL PROCEDURES.....	11
3.1 Periodontal diseases.....	11
3.2 Diagnosis of periodontal diseases.....	12
3.3 Treatment of periodontal diseases.....	15
3.4 Learning periodontal procedures with haptics-based dental simulators.....	17
4 IMPLEMENTATION OF THE PERIODONTAL SIMULATOR	18
4.1 Overview.....	18
4.2 Implementation details.....	21
4.3 Graphical User Interface.....	27
5 USE OF THE PERIODONTAL SIMULATOR.....	32
5.1 Training session.....	32
5.2 Preliminary evaluation of the simulator.....	33
5.3 Results of the preliminary evaluation.....	38
5.4 Validation of the simulator realism.....	40
6 CONCLUSIONS.....	42
6.1 Future research and development.....	42
CITED LITERATURE	44
VITA	46

LIST OF FIGURES

<u>FIGURE</u>	<u>PAGE</u>
Figure 1 Endoscopy Simulator.....	4
Figure 2 Endovascular Simulator.....	4
Figure 3 Hysteroscopy Simulator	4
Figure 4 Laparoscopy Simulator.....	4
Figure 5 Vascular Access Simulator.....	5
Figure 6 Cholecystectomy Simulator.....	5
Figure 7 DentSim.....	6
Figure 8 Image Guided Implantology.....	7
Figure 9 Dental Simulator Unit plus.....	7
Figure 10 DentSim at the University of Cardiff, Wales, UK.....	8
Figure 11 Novint Dental Smulator.....	9
Figure 12 Iowa Dental Surgical Simulator	9
Figure 13 SimuLife Simulator	10
Figure 14 Tooth anatomy.....	11
Figure 15 Periodontal probe.....	12
Figure 16 Healthy tissues.....	13
Figure 17 Periodontitis I	13
Figure 18 Periodontitis II.....	14
Figure 19 Periodontitis III.....	14
Figure 20 Scaling	15
Figure 21 Planning.....	15

LIST OF FIGURES (continued)

<u>FIGURE</u>	<u>PAGE</u>
Figure 22 Periodontal scaler	16
Figure 23 Periodontal explorer	16
Figure 24 Overview of the implementation of the periodontal simulator	18
Figure 25 Implementation details of the graphics and haptics rendering processes.....	22
Figure 26 Virtual periodontal probe	23
Figure 27 Virtual scaler	23
Figure 28 Virtual explorer	23
Figure 29 Measuring pocket depth with periodontal probe	28
Figure 30 Calculi being removed with scaler	29
Figure 31 Periodontal probe and one of its templates.....	30
Figure 32 Control panel	31
Figure 33 Validation of the periodontal simulator at UIC	33
Figure 34 Question 1.....	35
Figure 35 Question 2.....	35
Figure 36 Question 3.....	36
Figure 37 Question 4.....	36
Figure 38 Question 5.....	37
Figure 39 Question 6.....	37
Figure 40 Question 7.....	38

LIST OF ABBREVIATIONS

3D	Three dimensional
CAT	Computer Assisted Tomography
CRT	Cathode Ray Tube
DOF	Degrees Of Freedom
FLTK	Fast Light ToolKit
FLUID	Fast Light User-Interface Designer
GHOST	General Haptic Open Software Toolkit
GLUT	OpenGL Utility Toolkit
GROK	Graphical Representation of Knowledge Lab
GUI	Graphical User Interface
Hz	Hertz
IDSS	Iowa Dental Surgical Simulator
IGI	Image Guided Implantology
IOM	Institute Of Medicine
PICC	Peripherally Inserted Central Catheters
UIC	University of Illinois at Chicago
VR	Virtual Reality
VRDTS	Virtual Reality Dental Training System
VRML	Virtual Reality Modeling Language

SUMMARY

The haptics-based virtual reality periodontal training simulator project focuses upon the research and development of a prototype dental simulator for training of periodontal procedures. By the use of virtual reality and haptics technology, the periodontal simulator allows trainees to learn performing diagnosis and treatment of periodontal diseases by visualizing a three-dimensional virtual human mouth and feeling real tactile sensations while touching the surface of teeth, gingiva, bone and calculi with virtual dental instruments.

Since periodontics requires dentists to depend primarily on tactile sensations to perform diagnostic and surgical procedures, the use of haptics is unquestionably crucial for a realistic periodontal simulator.

The haptics-based virtual reality periodontal training simulator has been validated by experiments conducted by the College of Dentistry with faculty members and dental students, which demonstrates the scientific contribution and usefulness of the simulator as a vital part of the curriculum of the Department of Periodontics at UIC.

1 INTRODUCTION

The use of medical simulators has proved to increase patient safety and reduce risk associated with human errors in hospitals by allowing medical students to develop skills more efficiently in a shorter period of time. Even though medical simulators are currently being developed by a large number of universities and medical companies, the field of dental simulation has not been well exploited yet. This thesis focuses on the research and development of a haptics-based dental simulator specially designed for training and performance evaluation of dental and hygiene students and practicing professionals in Periodontics. The simulator is the result of a multidisciplinary project developed by the *Electronic Visualization Laboratory* of the Department of Computer Science, the *Industrial Virtual Reality Institute* of the Department of Mechanical and Industrial Engineering, and the Department of Periodontics at the University of Illinois at Chicago. The goal of this collaboration between the College of Engineering and the College of Dentistry at UIC is the implementation of a dental simulator to help increase the quality of training for students and future practitioners in the field of periodontics. The simulator allows trainees to develop the skills needed to differentiate pathological and normal conditions, as well as to diagnose and treat periodontal diseases. Trainees can learn by feeling tactile sensations as they “touch” a computer-generated 3 dimensional (3D) model of a human upper and lower dental arches along with various oral components: teeth, gingiva and bone with a haptic device. The simulator also facilitates the learning of proper selection and manipulation of dental instruments to perform periodontal procedures.

This thesis is organized in six chapters. Chapter 2 presents an overview of the current commercially-available medical simulators, followed by manikin-based and haptics-based dental simulators previously developed. Chapter 3 gives background information about the diagnosis and treatment of most common periodontal diseases and proposes the use of haptics-based dental simulators to facilitate the learning of these activities. Chapter 4 shows the implementation details and the graphical user interface of the virtual reality periodontal simulator. Chapter 5 describes the use of the simulator for periodontal training, and reports the results obtained after its validation by the College of Dentistry at UIC. Finally, chapter 6 outlines the conclusions of this work and suggests future research and development.

2 BACKGROUND

In the last decade, medical simulation has become a valuable learning and practicing tool for acquiring skills that were, until recently, performed by practice on laboratory animals, cadavers and even on living humans. Animals do not have the same anatomy as human beings, are expensive, and they are not reusable. Cadavers have the correct anatomy, but they are expensive, difficult to procure, and present some tissue degradation problems. On top of that, ethical issues are raised in both cases.

Simulation-based medical training provides an enhanced clinical skill development that benefits, not only patients but also health care consumers. According to [IOM, 1999] from 44,000 to 98,000 patients die each year as a result of “medical errors”, causing an estimated cost to the US economy of \$17 - \$29 billion dollars. Medical simulation improves health outcomes, patient safety and quality, reduces medical errors and deaths, and increases healthcare cost savings.

Common medical procedures, such as laparoscopy, colonoscopy, lung biopsy, vascular access and cardiovascular catheterizations, can be performed on physical manikins and computer-based simulators to train medical professionals without putting real patients in risky situations. Previous studies [Rowe et al. 2000] [Mehta et al. 2000] [Datta et al., 2001] [Wong et al. 2001] indicates that training on simulators has significantly improved students’ skill and performance on patients when compared to those individuals not trained on these devices.

2.1 Medical simulators

One of the best known companies that currently offers medical simulators is [Immersion Technology], which commercializes a series of simulators for minimally

invasive medical procedures (such as vascular access, endoscopy, endovascular, hysteroscopy and laparoscopy) that provide users both cognitive and psychomotor skills.

Immersion's AccuTouch[®] medical simulator product line consists of five platforms:

- **Endoscopy simulator:** Bronchoscopy and upper and lower gastrointestinal procedures on a single platform (Figure 1)



Figure 1

- **Endovascular simulator:** Percutaneous coronary and peripheral interventions and cardiac rhythm management (Figure 2)



Figure 2

- **Hysteroscopy simulator:** Skills assessment and myomectomy (Figure 3)

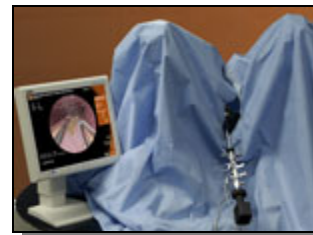


Figure 3

- **Laparoscopy simulator:** Skills assessment, cholecystectomy, sterilization, ectopic pregnancy, and myomectomy suturing (Figure 4)



Figure 4

- **Vascular access simulator:** Procedure Training, Anatomical Viewer, Single Cases, and Career Mode instruction modules; and Peripherally Inserted Central Catheters (PICC) (Figure 5)



Figure 5

Another company is [Reachin Core Technology] that offers a haptics-based simulator for training on a particular laparoscopic surgery called cholecystectomy, which consists of the removal of the gall bladder. (Figure 6)



Figure 6. Cholecystectomy Simulator

2.2 Dental simulators

Even though complex and realistic medical simulators are becoming more and more common in medical education, the use of simulators in the field of dentistry has not been well exploited yet. Dental simulators provide an efficient way to quickly teach preclinical dental students on dental procedures while increasing their hand skills considerably. Repetitive procedures such as proper hand and instrument usage and placement are primary targets to be learned on dental simulators.

There are two kinds of dental simulators currently available: **manikin-based simulators** that provide a physical model of the patient's head and mouth on which certain dental procedures can be performed using real dental instruments; and **haptics-based simulators** that employ a PHANTOM™ haptic device [SensAble Technologies, Inc] and virtual models of a human tooth or mouth as a platform to facilitate dental practicing. Instead of using real dental instruments, the trainee holds the haptic device stylus to manipulate a set of virtual instruments that are shown on a monitor screen. The tactile feedback reproduces clinical sensations in the hand of the operator using dental instruments.

2.2.1 Manikin-based dental simulators

There are two companies that commercialize similar manikin-based dental simulators worldwide: DenX and KaVo.

- DentSim™, developed by [DenX Ltd], consists of a manikin with head and dentoform (plastic teeth), a dental hand-piece and a light, an infrared camera and two computers. The manikin head and the hand-piece contain infrared emitters that are tracked by the infrared camera. Using this optical tracking system to trace the movements of a hand piece, the simulator scores the accuracy of a student's cavity preparation in a manikin's synthetic tooth. (Figure 7)



Figure 7

- Image Guided Implantology (IGI), also developed by DenX, Ltd, uses the same technology of DentSim™ for teaching, diagnosis, treatment planning and placement of implants. Providing a particular patient's CAT scan, the simulator allows the patient and the virtual model image to be coordinated during the actual surgery. If the computer recognizes that the surgeon is making a serious deviation from the treatment plan during the actual surgery, the computer will stop the hand-piece and the surgeon will need to override the computer to continue. (Figure 8)



Figure 8

- Dental Simulation Unit plus (DSEplus), commercialized by [KaVo], is a complete training unit with pneumatic chassis, storage space, supply unit, pressurized water module, suction module, dentist's element with instrument tubes and 3-F syringe, assistant's element with 2 suction tubes, foot control, patient simulator, cranium with jaws, tooth model, face mask and pneumatic patient positioning system. (Figure 9)

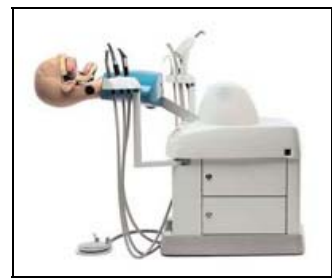


Figure 9

The use of manikin-based dental simulators, compared to the traditional preclinical methods, increases the educational outcomes according to [Buchanan, 2001,

2004]. [Jasinevicius et al., 2004] found that even the instruction time spent by faculty is decreased when using DentSim™ simulators. In addition, a higher number of students can be trained on technical skills at the same time, because the traditional time-consuming one-to-one relationship between the student and the instructor is not required any more [Chan et al., 2000].

Figure 10 shows an example of a deployment of DentSim simulators at the University of Cardiff, Wales, UK.

However, those simulators present the following disadvantages:

- A physical model or manikin needs to be frequently replaced, increasing the maintenance costs considerably.
- They do not provide any indications if the treatment performed by the student would be potentially aggressive for a real patient.



Figure 10. DentSim at the University of Cardiff, Wales, UK

2.2.2 Haptics-based dental simulators

Unlike manikin-based, haptics-based simulators are much more cost effective because no physical models need to be replaced. In addition, since the haptic device measures the forces applied by the trainee when touching the virtual patient's mouth, it is possible to detect when the trainee's performance is too aggressive.

The followings are some of the most well-known haptics-based dental simulators previously developed:

- Virtual Reality Dental Training System (VRDTS) was developed by [Novint Technologies] in collaboration with the Harvard School of Dental Medicine. Aiming for cavity preparation, the software simulates a set of dental instruments (low speed drill, an explorer, two carvers, a carrier and a packer), amalgam material, and a single molar including enamel, dentin, caries and pulp materials. (Figure 11)



Figure 11

- Iowa Dental Surgical Simulator [IDSS] was a joint project between the College of Dentistry at the University of Iowa and the Graphical Representation of Knowledge (GROK) Lab. Participants can feel enamel, healthy dentin and carious dentin as touching the virtual tooth. (Figure 12)

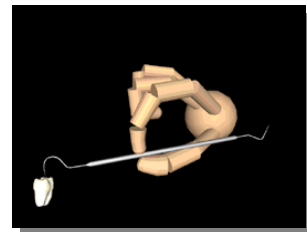


Figure 12

- 3DDental, commercialized by [SimuLife, 2002], provided tactile feedback to reproduce clinical sensations (such as probing caries, drilling and filling of cavities) in the hand of the operator using a virtual explorer or a drill. 3DDental simulator is no longer available. (Figure 13)



Figure 13

Even though the previous haptics-based dental simulators have proven to be successful in the simulation of restorative dentistry such as caries preparation or filling of cavities, none of them focuses on the simulation of periodontal procedures. Unlike previous developments, this haptics-based dental simulator was designed especially for periodontics¹. This field of dentistry requires dentists to depend primarily on their tactile sensations, for both diagnostic and surgical procedures. This makes haptics ideally suited for periodontal simulators.

¹ A preliminary implementation of the UIC periodontal simulator, with a single tooth, was developed by [Montanari, 2002] in an early stage of this project [Steinberg, 2003].

3 PERIODONTAL PROCEDURES

3.1 Periodontal diseases

Periodontal diseases are bacterial gum infections that destroy the attachment fibers supporting bone that hold teeth in place. The main cause of periodontal diseases is bacterial plaque. If plaque is not removed, it can turn into a hard substance called calculus in less than 2 days. If calculus forms below the gum line, on the root of the tooth, it makes plaque removal more difficult, possibly causing a periodontal disease.

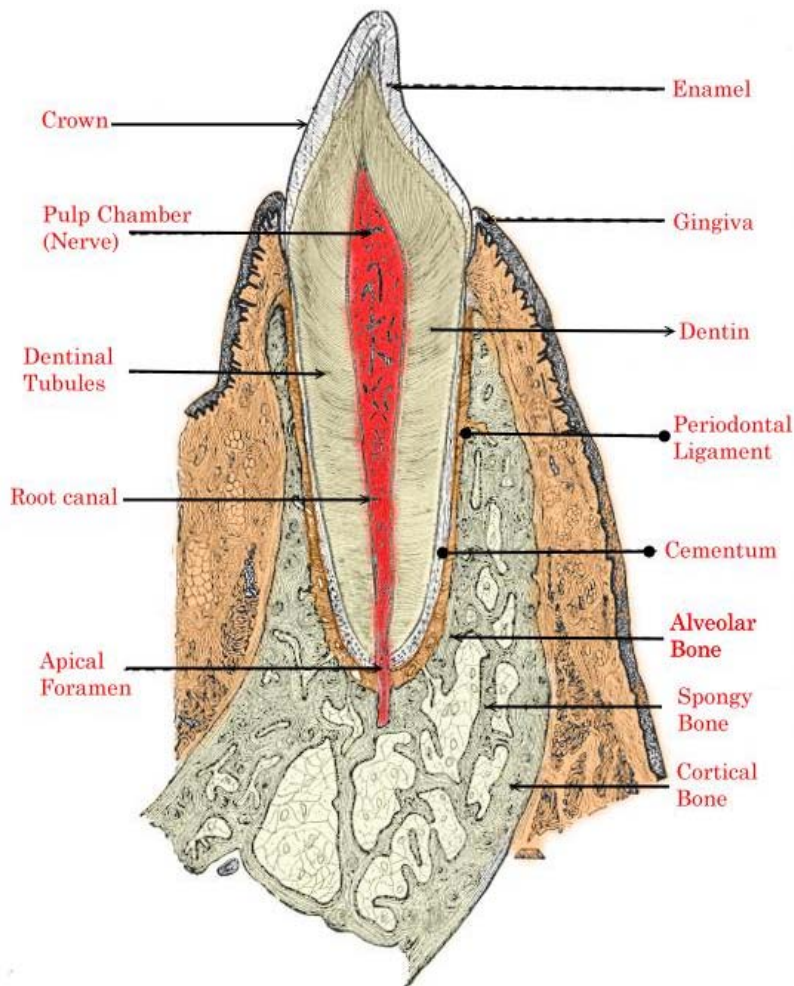


Figure 14. Tooth anatomy [Spiller]

Toxins produced by the bacteria in plaque irritate the gingiva (gums), causing infection that can destroy the supporting tissues around the teeth, including the bone. Figure 14 shows the anatomy of a tooth and its supporting structure. When this happens, gums separate from the teeth, forming pockets that fill with even more plaque and more infection. As the disease progress, these pockets deepen, more gum tissue and bone are destroyed, and the teeth eventually become loose. If periodontal diseases are not treated, the teeth may need to be removed. [Racine Dental Group]

3.2 Diagnosis of periodontal diseases

Periodontitis is diagnosed by the use of a periodontal probe (Figure 15), which is a depth measurement device. With very little pressure, the probe is slipped down next to the root of the tooth until there is a resistance. The markings shown on the instrument demonstrates the depth of the gum pocket (in millimeters).

The severity of the periodontal disease is measured according to the depth of the gum pocket. The following table shows a comparison of the possible cases of periodontitis and their related symptoms [Enexus] [Hafernik].



Figure 15. Periodontal probe

Healthy tissues

No bleeding or puffy gums, all normal pockets measure 3mm or less. (Figure 16)

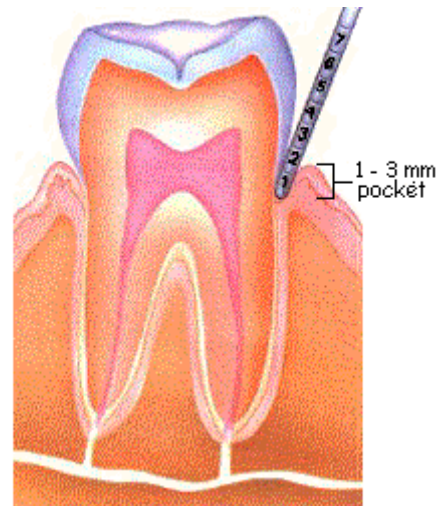


Figure 16

Periodontitis I (Gingivitis)

Bleeding gums when measured, puffy in appearance and pockets no greater than 3mm. No damage to the supporting bone in this stage. (Figure 17)

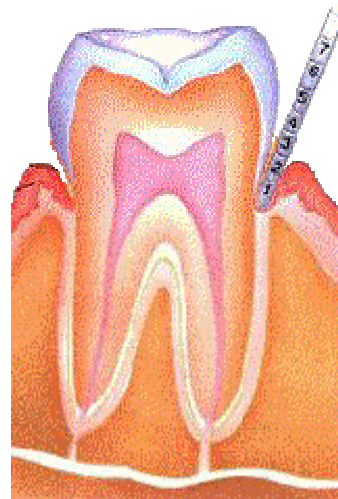


Figure 17

Periodontitis II

Bleeding and puffy gums that measure slightly more than normal at up to 5mm.

(Figure 18)

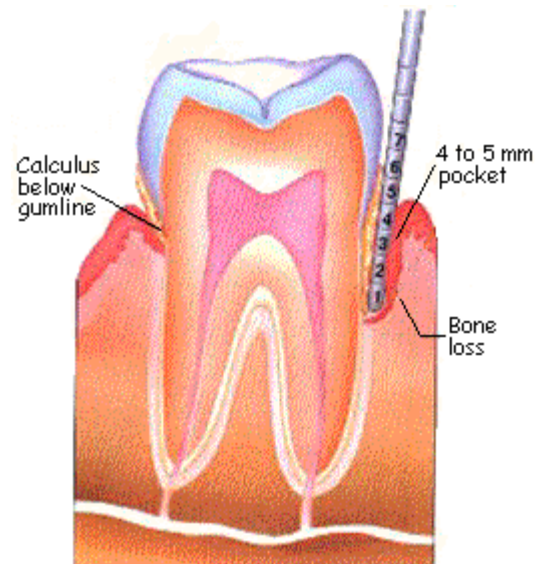


Figure 18

Periodontitis III

Bleeding and swollen gums with pockets that measure up to 6mm and more. Bone recession beginning to appear.

(Figure 19)

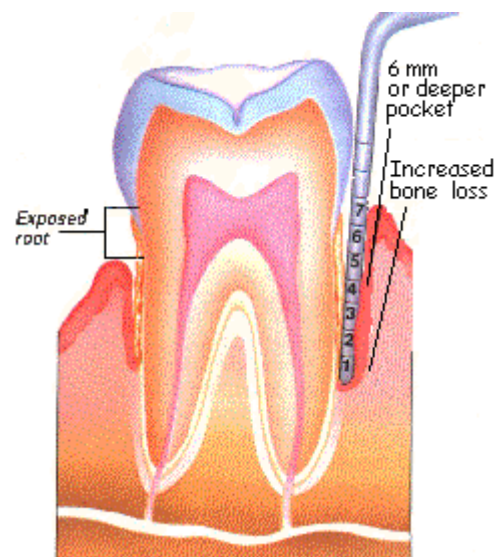


Figure 19

3.3 Treatment of periodontal diseases

Treatment for all stages of a periodontal disease involves the thorough removal of all plaque and calculus that has adhered to the teeth. This can be removed during a normal prophylaxis without too much discomfort on the part of the patient. When the damage from gum disease is slight, this can be done without local anesthesia. The process is called "**scaling**". (Figure 20)

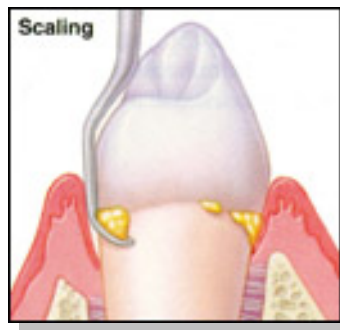


Figure 20. Scaling [Peterson]

When the damage from periodontal disease is more pronounced, exposing more root structure above bone, the process is called "**root planning**" (Figure 21). Root planning always requires local anesthesia. The root of a tooth is naturally sensitive, and that is why local anesthesia may be needed when working in this area [Spiller] [Peterson].

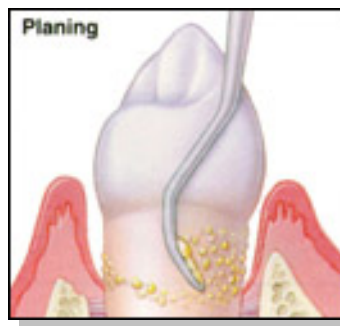


Figure 21. Planning [Peterson]

Scaling and root planning are performed using a dental instrument called periodontal scaler (Figure 22), which removes plaque and calculus from below the gum line. This controls the growth of destructive bacteria, and helps the gums to reattach to the root of the tooth.

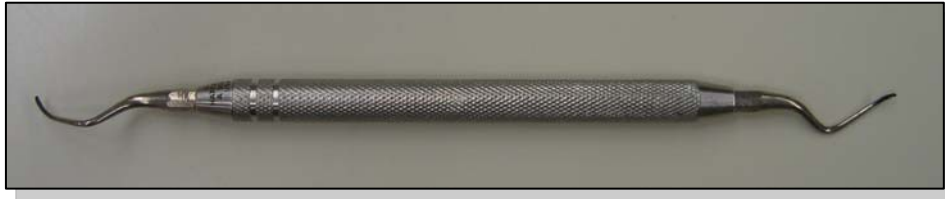


Figure 22. Periodontal scaler

As a final procedure, a periodontal explorer (Figure 23) is used to determine by the sense of touch whether the scaled root surface has the calculus removed and has been properly instrumented. The periodontal explorer is also used to evaluate the area of the root surface covered by the gingiva to assess for the presence of dental caries on the root surface, assess abnormalities in root morphology and evaluate the presence of improperly finished dental restorative margins.

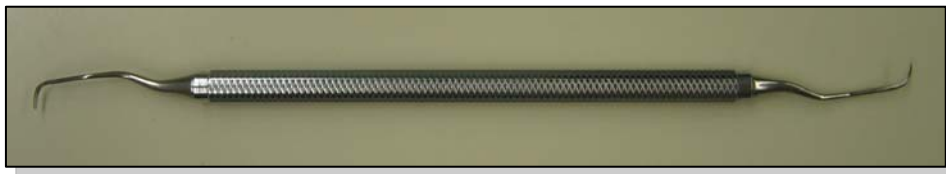


Figure 23. Periodontal explorer

3.4 Learning periodontal procedures with haptics-based dental simulators

Currently in Dental Schools, periodontal procedures are taught by instructor demonstration, use of practice manikins and, finally, by actual work in the patient's mouth. This time consuming teaching process requires excessive one-on-one instructor/student interaction. Haptics-based dental simulators could facilitate the training of dental and hygiene students in these periodontal procedures. They should aid in diminishing the instruction time period, enhance the learning curve and provide for unlimited practice of these treatments.

In the diagnosis phase, a virtual periodontal probe could be used to measure pocket depth and determine the tissue health and, in case of pathological situations, the severity of the periodontitis.

In the treatment phase, a virtual periodontal scaler could be used to detect the presence of calculus. With the tooth surface covered by gingiva, the trainee would be forced to rely on the tactile sensation obtained from the haptic device to evaluate the presence of virtual calculus on the root surface. Showing a transparent gingiva, the trainee could concomitantly see the calculus under the gum line.

In the evaluation phase, a virtual periodontal explorer may be used to determine that the calculus has been completely removed. This evaluation could be performed with both a transparent and an opaque gingiva to contrast the results obtained by the trainee.

4 IMPLEMENTATION OF THE PERIODONTAL SIMULATOR

4.1 Overview

Figure 24 shows the top level of the implementation of the haptics-based periodontal simulator. The user interacts with the simulator via a stereoscopic display and a haptic device. The stereoscopic display consists of a CRT monitor, capable of a vertical refresh rate superior to 100 Hz, synchronized with a pair of Crystal Eyes active stereo shutter goggles from [StereoGraphics]. The haptic device is a [SensAble] 6-DOF (output) and 3-DOF (input) PHANToM Desktop.

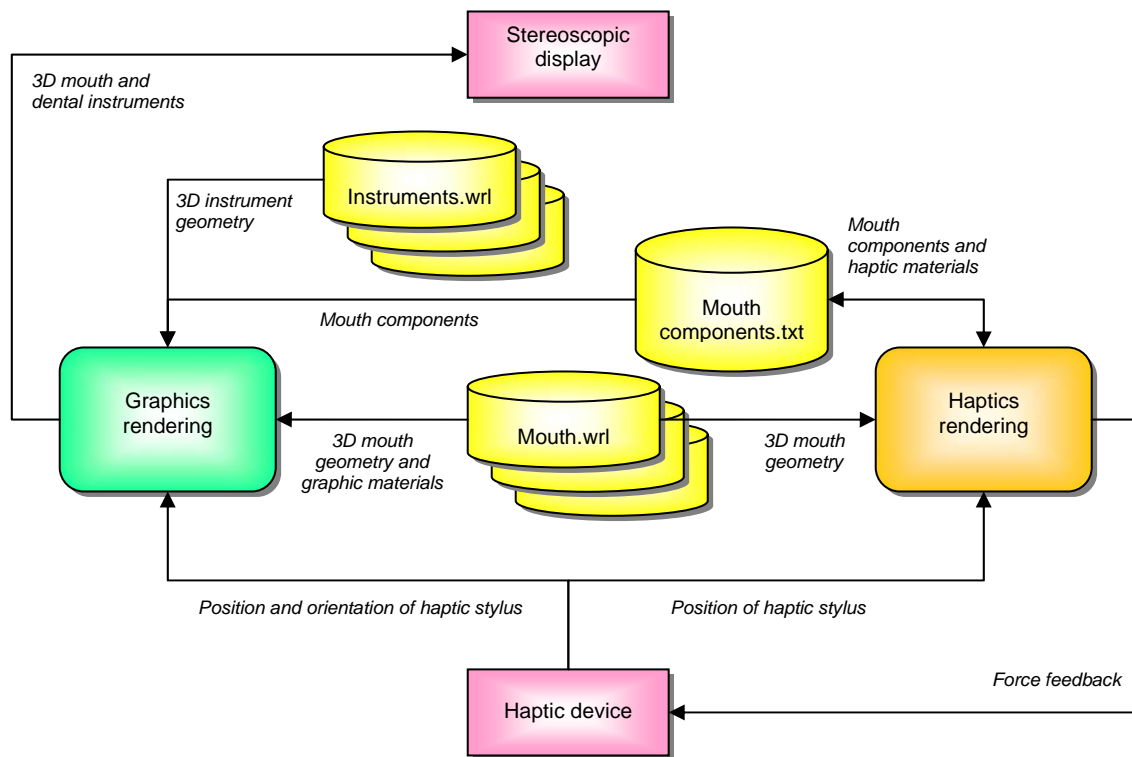


Figure 24. Overview of the implementation of the periodontal simulator

The simulator has been organized as basically two processes that run concurrently in two different threads on a Windows platform:

- Graphics rendering
- Haptics rendering.

The graphics rendering has been developed on top of Coin, a high-level 3D graphics library that uses scenegraph data structures to render real-time computer graphics. Coin is an open-source implementation of Open Inventor by [Systems in Motion], ideal to develop scientific and engineering visualization applications. The graphics rendering process is in charge of the stereo visualization of the 3D virtual mouth, dental instruments and templates. Coin traverses the scenegraph twice: once for the left view and once for the right view. Using the quad buffer in the graphics card, Coin stores both views in two different frame buffers, which are then displayed by the CRT in synchronism with the shutter goggles.

The haptics rendering has been developed on top of GHOST (General Haptic Open Software Toolkit), which is a cross-platform haptics library commercialized by [SensAble Technologies] for its PHANToM haptic devices. The haptics rendering reads the current status of the haptic device, detects the collisions between the virtual dental instruments and the virtual mouth, and computes the reaction forces to be applied by the haptic device.

Both processes traverse different scenegraph trees stored in memory at different frame rates. While the graphics scenegraph is rendered on the stereoscopic display at 60 Hz (30 Hz for each left and right views in active stereo mode), the haptics scenegraph is

rendered on the haptic device at 1000 Hz to avoid undesired system instabilities that can be felt as vibrations or force discontinuities.

The simulator stores and reads information to and from three files:

- “Mouth.wrl”
- “Mouth components.txt”
- “Instruments.wrl”

“Mouth.wrl” is a set of VRML files containing the 3D geometry (vertices and faces) and their graphic materials (diffuse, ambient and specular coefficients). The 3D model of the mouth was originally purchased from the Viewpoint 3D model catalog [by Digimation], manipulated with 3DStudioMax 6.0 [by Autodesk] for a more efficient real-time graphics and haptics rendering, and then exported as VRML files.

“Mouth components.txt” is an ASCII file containing a list of 3D objects that form the virtual mouth: tooth roots, tooth crowns, gingiva, bone and calculi. For each component, the file contains the following fields:

- Name of VRML file associated to the 3D component (“mouth.wrl”)
- Stiffness coefficient (spring)
- Viscosity coefficient (damper)
- Static friction coefficient
- Dynamic friction coefficient
- Enabled or disabled haptics

Finally, “Instruments.wrl” is also a set of VRML files describing the 3D geometry and graphic materials of the three virtual dental instruments needed for the periodontal

procedure: a periodontal probe, a scaler and an explorer. The 3D virtual instruments were modeled using 3DStudioMax 6.0 and then exported as VRML files.

4.2 Implementation details

Figure 25 shows the graphics and haptics rendering processes in more detail. All processes shown in green are sub-processes of the graphics rendering, whilst the ones shown in orange correspond to the haptics rendering. Note that in addition to the stereoscopic display and the haptic device, the keyboard and mouse have been added to the diagram to describe the complete user interaction. All sub-processes are described as follows:

1. Read 3D mouth for graphics rendering:

This process reads the filenames of the 3D objects listed in the “mouth components.txt” file. That information serves as a link to the set of “mouth.wrl” files that store the 3D geometry and the graphic materials of the teeth, gingiva, bone and calculi as VRML nodes.

2. Visualize 3D mouth

The sub-scenegraph containing the mouth components is added to the main scenegraph to be rendered by Coin.

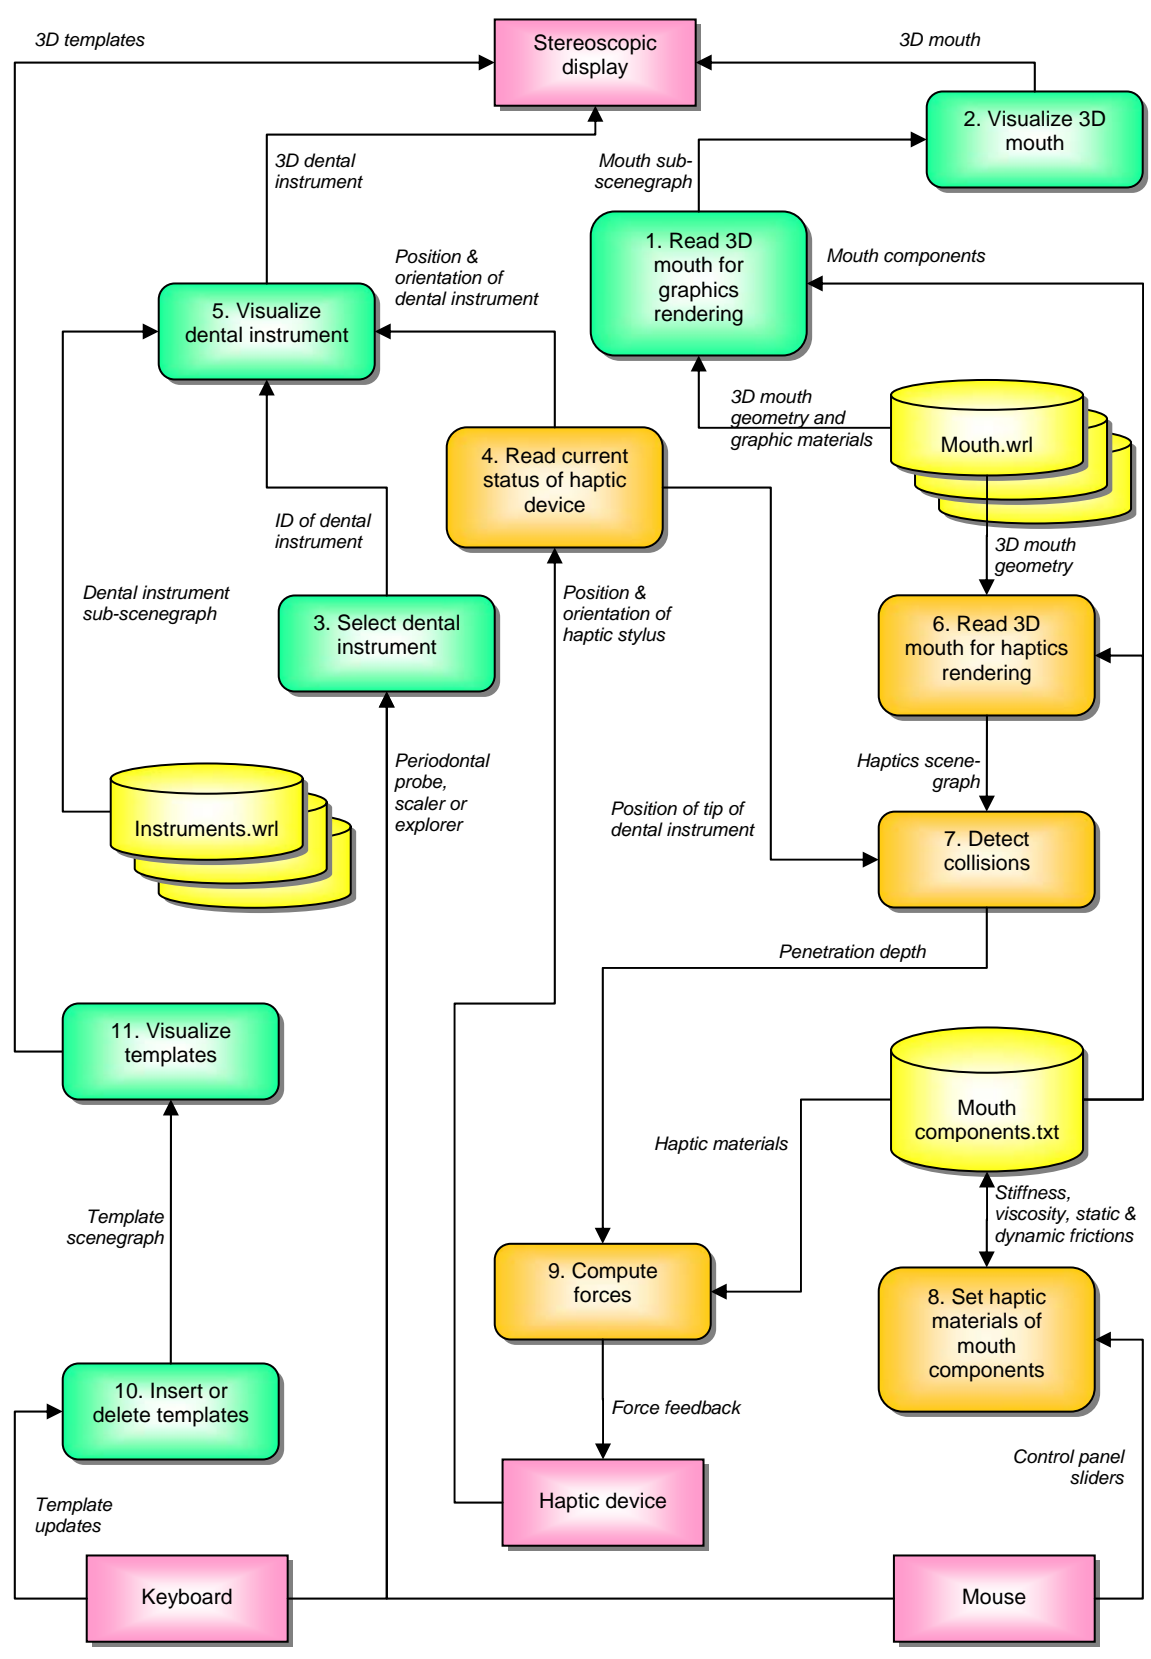


Figure 25. Implementation details of the graphics and haptics rendering processes

3. Select dental instrument

Since each periodontal procedure requires the use of different dental instruments for diagnosis and for treatment of the periodontal disease, the user can select one of the three virtual instruments simply pressing the following “hot” keys:

- “p” for periodontal probe (Figure 26)
- “s” for scaler (Figure 27)
- “e” for explorer (Figure 28)

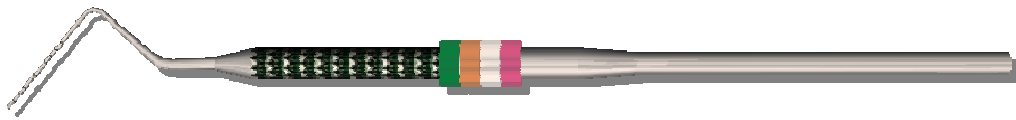


Figure 26. Virtual periodontal probe



Figure 27. Virtual scaler



Figure 28. Virtual explorer

4. Read current status of haptic device

GHOST computes the inverse kinematics [Craig, 1986] to determine the position and orientation of the haptic stylus from the information given by the encoders attached

to each servomotor of the haptic device. The position and orientation of the stylus held by the user define the translation and rotation transformation applied to the virtual dental instrument in the 3D virtual environment.

5. Visualize dental instrument

The 3D geometry and graphic materials of all virtual instruments stored in the “instruments.wrl” files are added to the graphics scenegraph. However, only the chosen instrument is rendered. The user manipulates the haptic stylus as s/he would do it with a real dental instrument, while the 3D representation of the chosen virtual instrument is displayed on the screen in stereo.

6. Read 3D mouth for haptics rendering

This process also reads the list of objects from the “mouth components.txt” file. Thanks to certain compatibility with VRML format, GHOST is also able to import the 3D geometry from the set of “mouth.wrl” VRML files to store a haptics scenegraph in main memory. Recall that even though the haptics scenegraph (for GHOST) and the graphics scenegraph (for Coin) contain the same 3D objects, they are concurrently traversed at different frame rates by different libraries.

7. Detect collision

The position of the haptic device allows GHOST to compute a point-based collision detection between the tip of the virtual dental instrument and the 3D teeth, gum, bone and calculi previously added to the haptics scenegraph. The penetration depth, which is the 3D vector from the surface contact point and the current position of the

virtual probe, is calculated by GHOST for all colliding objects in the scene to perform the haptics rendering.

8. Set haptic materials of mouth components

Since the VRML standard does not provide a way to define haptic materials, the “mouth components.txt” file is used to store four coefficients: stiffness (spring), viscosity (damper), static and dynamic frictions to define the property of the haptic materials of each 3D object. The user can define these coefficients in real time adjusting the sliders in the control panel.

9. Compute forces

GHOST implements a spring-damper model to compute reaction forces using the penetration depth of the virtual proxy and the haptic materials of the colliding object. The forces are then sent to the haptic device to give the user the illusion of “touching” the virtual mouth.

10. Insert or delete templates

The 3D orientation of the dental instrument with respect to the tooth is crucial to succeed in the diagnosis and treatment of a periodontal disease. Its ideal orientation depends on the location of the tooth surface that needs to be reached by the dental instrument. Because of its complexity, instrument approach is very cumbersome for the instructors to teach to dental students. Templates were incorporated to the periodontal simulator to facilitate that learning process. Templates are additional virtual instruments that are displayed in the virtual environment to guide dental students in the orientation of the dental instruments as certain way of “scaffolding”.

To add a new template, the instructor holds the haptic stylus in the desired position and orientation and then presses the <insert> key. A semi-transparent virtual instrument is then frozen in that particular location (Figure 31). The student can then rotate the virtual mouth to see the desired orientation from any viewpoint. Many templates can be added to the scene to show different conditions while performing the periodontal procedure.

Templates can be interactively removed from the scene by locating the tip of the stylus close to it and then pressing <delete> key.

Alternatively, templates can be added or deleted clicking on the respective control panel buttons.

11. Visualize templates

The scenegraph containing all templates is added to the main scenegraph to be rendered by Coin. The transparency of the templates can be adjusted in real time by the user via the control panel.

4.3 Graphical User Interface

The periodontal simulator GUI has been developed using the Fast Light ToolKit [FLTK], which is a small and modular freely-available cross-platform C++ GUI. It supports 3D graphics via OpenGL[®] and its built-in GLUT emulation. With FLTK it is possible to incorporate all of the usual widgets to develop applications (menus, buttons, sliders, etc.). It even has a Fast Light User-Interface Designer (FLUID), which is useful to easily draw the user-interface and to define functions, classes and variables as needed. FLUID creates C++ source and header files that can be included in the application.

Figure 29 shows how the user can measure the pocket depth with the markings of the virtual periodontal probe. Figure 30 displays a transparent gingiva to show the presence of calculi attached to two molars and how they can be removed by a virtual scaler during the simulation of the root planning. Figure 31 shows the correct position and orientation of the periodontal probe by the visualization of its template.

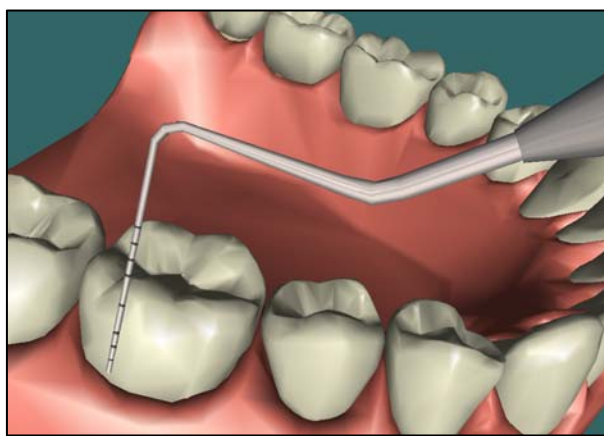
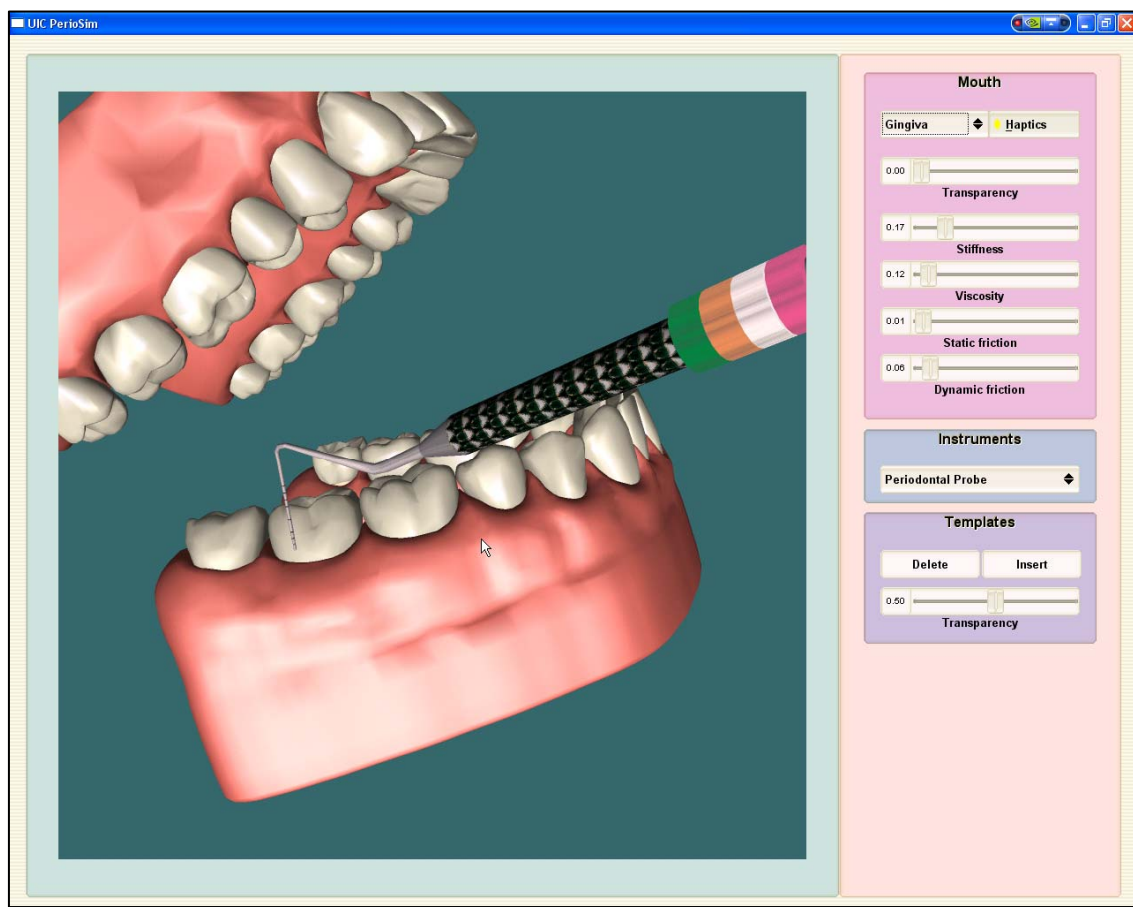


Figure 29. Measuring pocket depth with periodontal probe

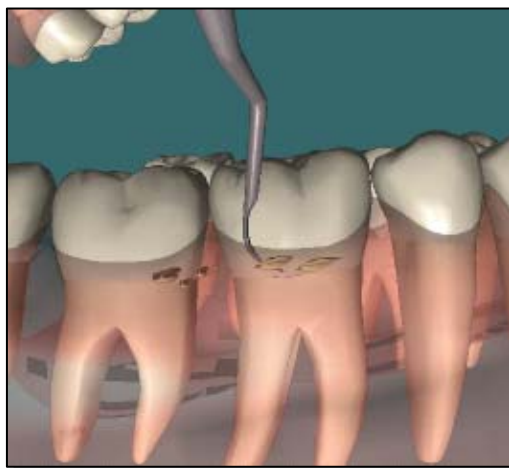
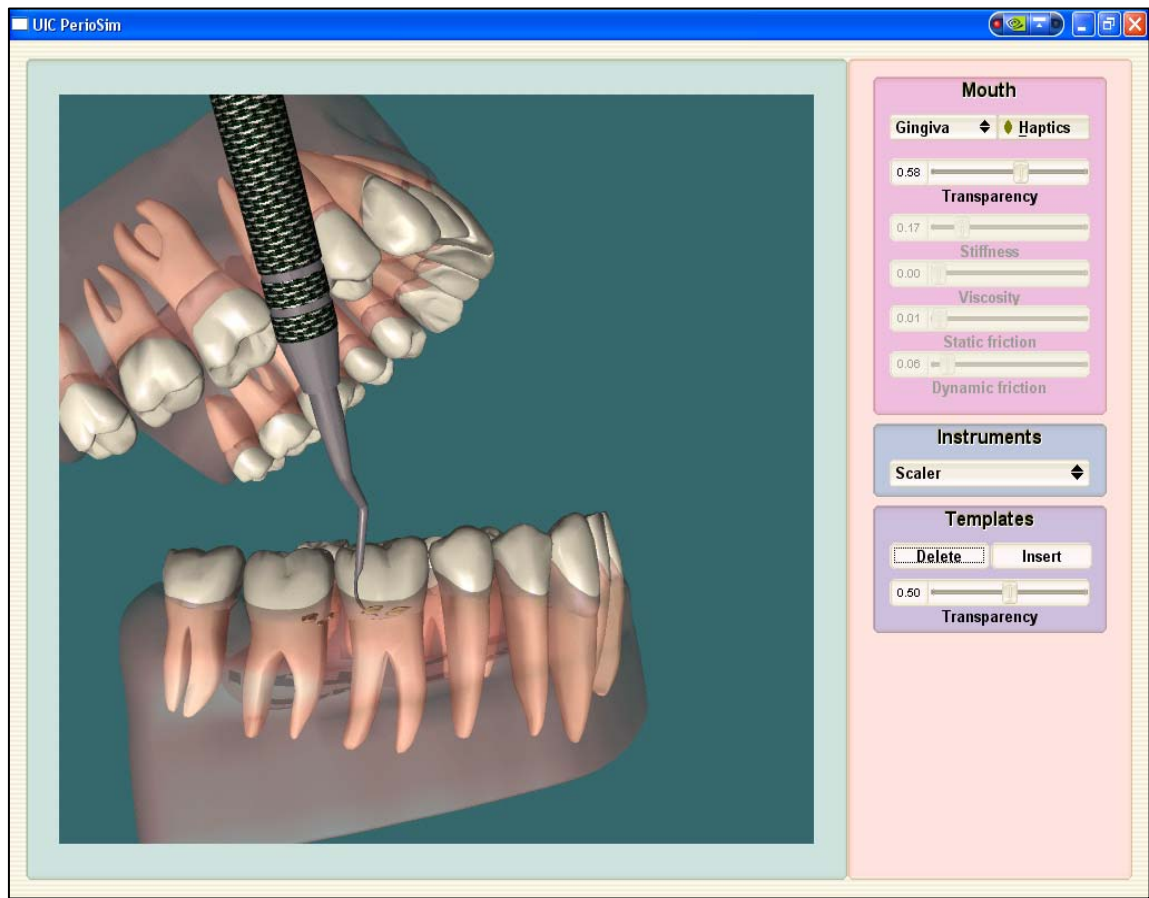


Figure 30. Calculi being removed with scaler

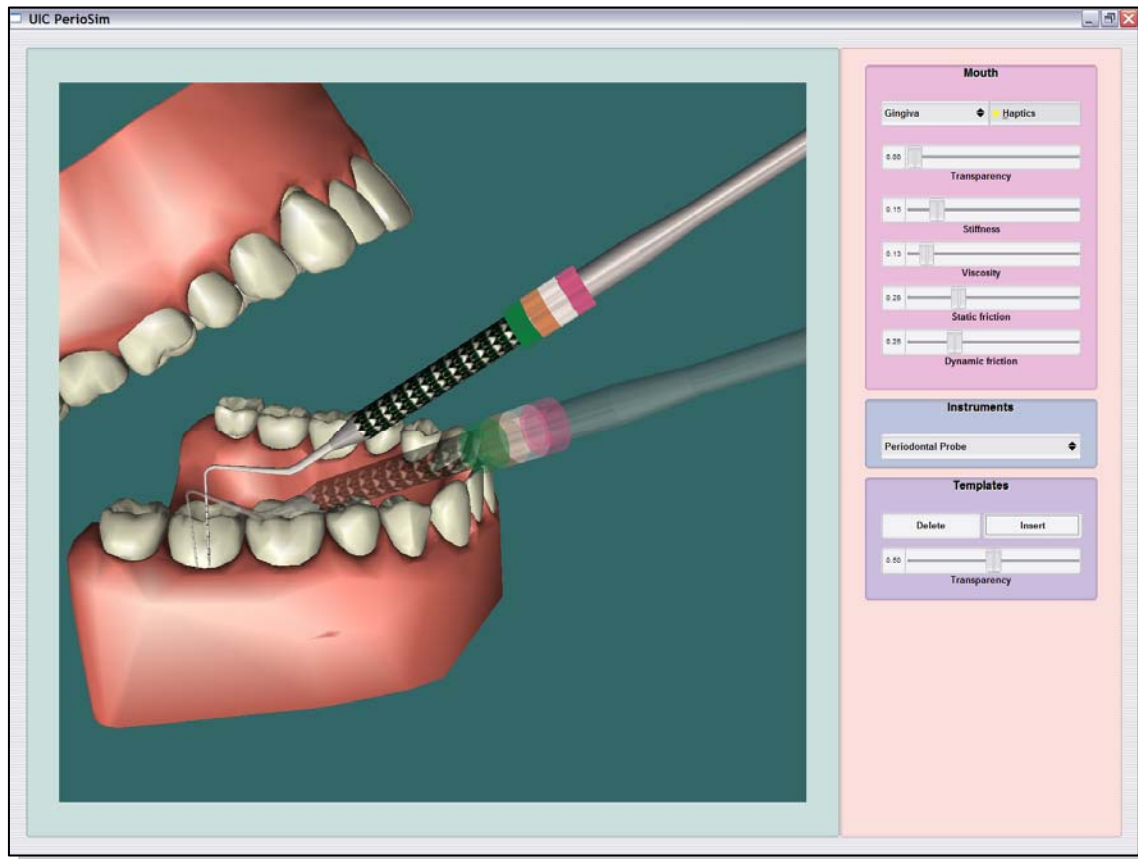


Figure 31. Periodontal probe and one of its templates

The control panel shown in Figure 32 has a variety of controls, including adjustment of the haptic feel by setting stiffness, viscosity, and static and dynamic friction coefficients, as well as the degree of transparency of the gingiva, roots, crowns, or calculus. The dental instrument can be selected by the control panel, which also permits the instructor to insert a variety of templates to guide the student to position the instrument correctly in a 3D display environment.

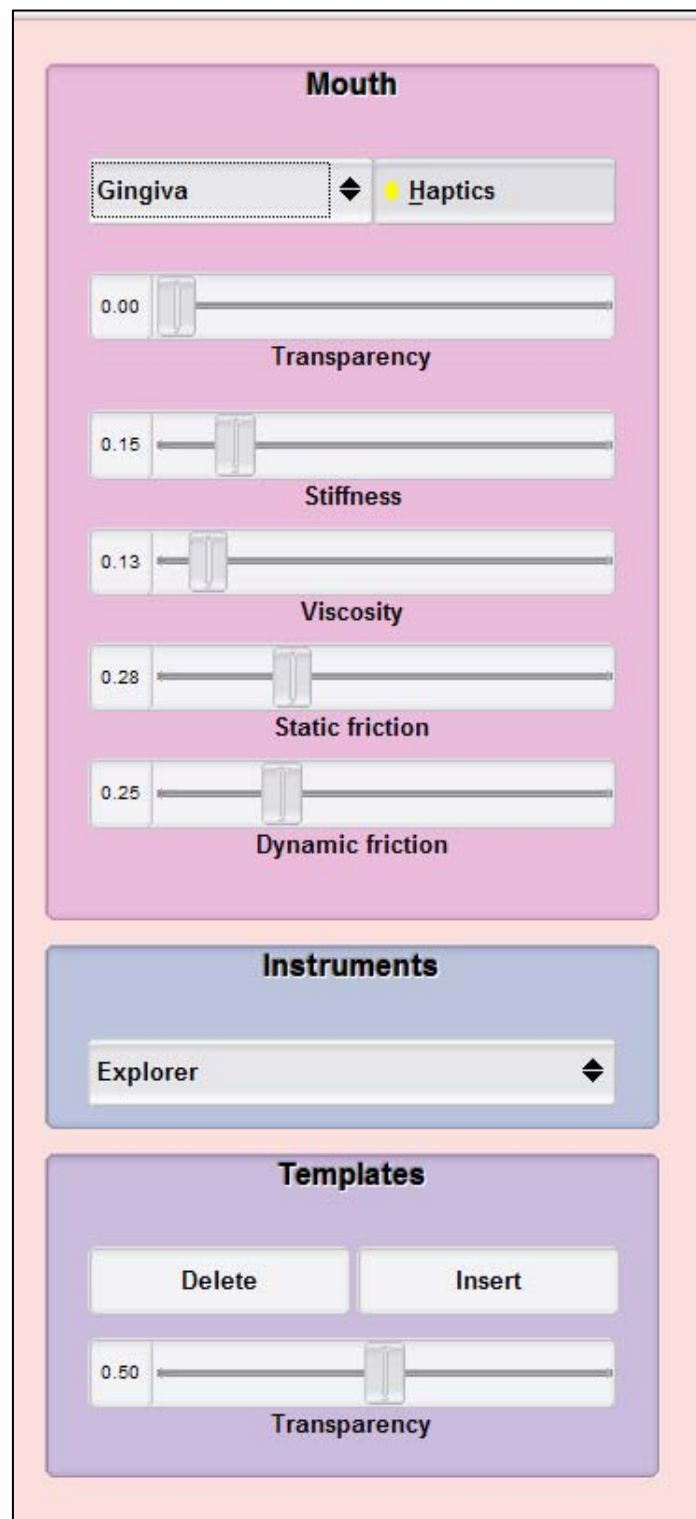


Figure 32. Control panel

5 USE OF THE PERIODONTAL SIMULATOR

5.1 Training session

The haptics-based dental simulator is currently being used by the Department of Periodontics at the University of Illinois at Chicago to train dental students in periodontal probing. The training session consists of the following steps. By moving the haptic controller device, a trainee can move and feel the VR instrument on the tooth surface or feel the crevice or pocket area within the margin of the gingiva (gums) along the root surface of the tooth. Using the control panel, one of three periodontal instruments can be selected for onscreen use: a periodontal probe, explorer or scaler. The 3D virtual periodontal probe can be used to locate and measure crevice or pocket depths around the gingival margins of the teeth.

A trainee can differentiate the textural feel of pocket areas and locate regions of sub gingival calculus. Since the root surface is covered by gingiva, the trainee cannot see the area being probed or the underlying calculus and must depend totally on haptic feedback to identify these areas. This situation corresponds to conditions encountered clinically. To assist visualization of what he/she is feeling, control panel adjustments can introduce varying degrees of gingival transparency.

Graphical and haptic parameters can be altered by an instructor using control panel adjustments to provide the “feeling” or feedback he/she wishes to impart to the trainee.

The system permits any instructor to generate a diagnostic and/or treatment procedure for student use. Recording of the haptic experiences involves the production of instructor driven trajectories to define correct movements of the dental instrument when

performing the periodontal procedure. These recordings can be stored in the system for future use by students and will guide their performance of a procedure. The methods used by an individual instructor to both diagnose and treat a particular procedure can be demonstrated while guiding students to perform the procedure in the same fashion. Note that the instructor need not be present to provide this guidance.

5.2 Preliminary evaluation of the simulator

Validation of the haptics-based periodontal simulator was conducted by the Department of Periodontics at UIC (Figure 33). A seven-question survey was obtained from 18 faculty members and 5 students of the College of Dentistry immediately after a 10-minute experience with the simulator [Dean's Report, 2004].

Three clinical instructors in the Department of Periodontics at UIC set the coefficients of the haptic materials to allow tactile differentiation between enamel, gingiva, crevicular or pocket areas and calculus.

The survey questions were answered in a 1-to-5 scale, where 1 corresponds to “strongly disagree” and 5 corresponds to “strongly agree”. Results of the experiment are shown below (third column of the table below shows the number of people that shared the same answer).



Figure 33. Validation of the periodontal simulator at UIC

Question		1	2	3	4	5		Mean
1. The Haptic Simulator was easy to use (Figure 34).	Strongly disagree	1	2	4	8	8	Strongly agree	3.9
2. The Haptic Simulator will be useful in teaching how to use the periodontal instruments shown and the tactile sensation that they relay (Figure 35).	Strongly disagree	0	2	2	7	12	Strongly agree	4.3
3. The Haptic Simulator would be a useful adjunct to the material provided in the regular class lectures and demonstrations (Figure 36).	Strongly disagree	1	0	1	6	15	Strongly agree	4.5
4. The short amount of time I engaged with the Haptic Simulator was sufficient to evaluate its effectiveness (Figure 37).	Strongly disagree	1	4	6	6	6	Strongly agree	3.5
5. The Haptic Simulator took too much time to use (Figure 38).	Strongly disagree	10	6	5	1	1	Strongly agree	2.0
6. The Haptic Simulator was useful in helping you feel how “live” periodontal tissue, tooth structure or calculus feels when using a periodontal instrument (Figure 39).	Strongly disagree	1	2	7	4	9	Strongly agree	3.8
7. The Haptic Simulator will be useful for course material review in the future (Figure 40).	Strongly disagree	0	1	3	8	11	Strongly agree	4.3

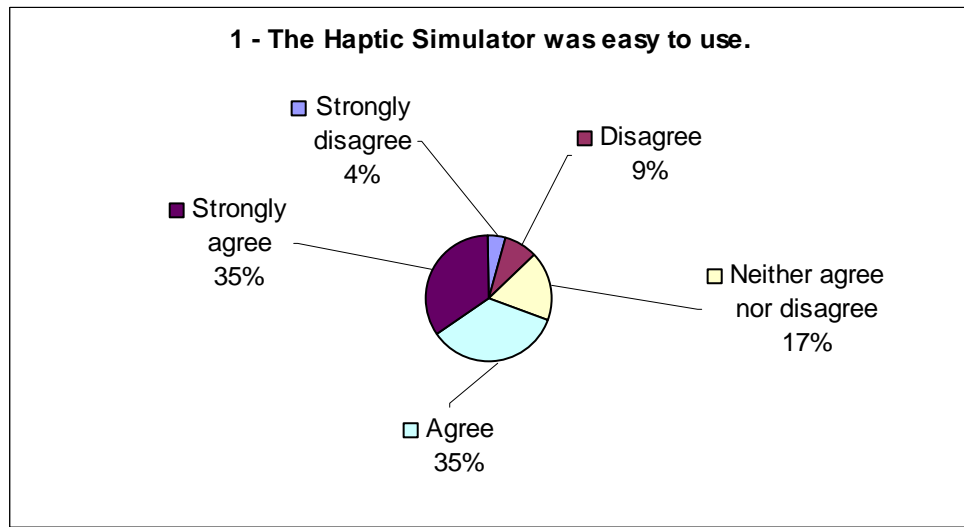


Figure 34. Question 1

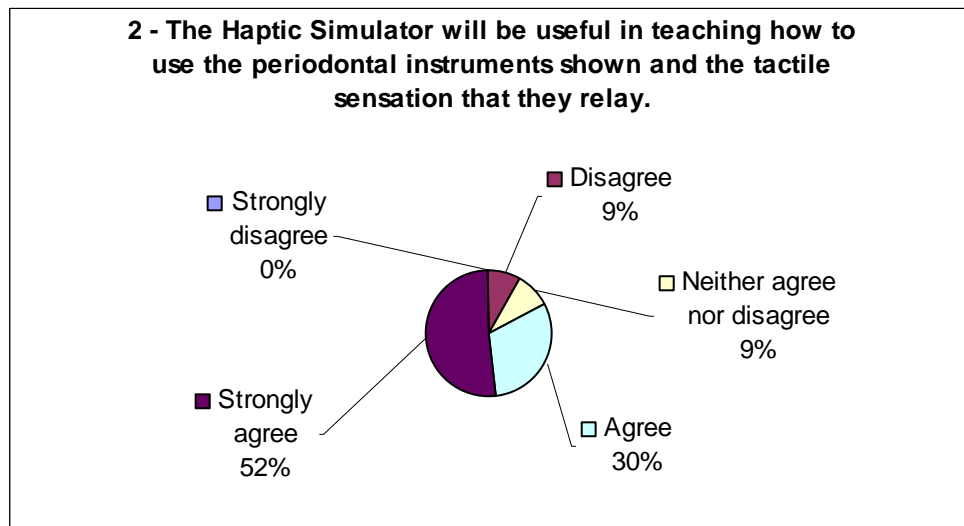


Figure 35. Question 2

3- The Haptic Simulator would be a useful adjunct to the material provided in the regular class lectures and demonstrations.

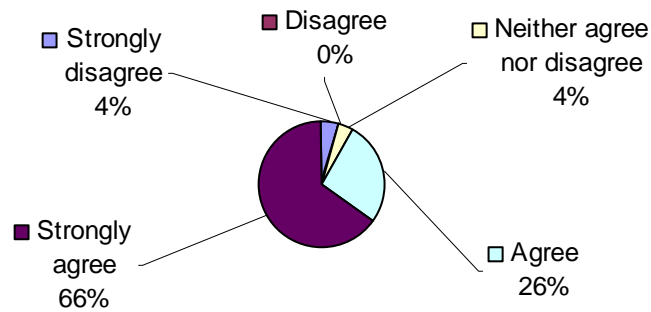


Figure 36. Question 3

4 - The short amount of time I engaged with the Haptic Simulator was sufficient to evaluate its effectiveness.

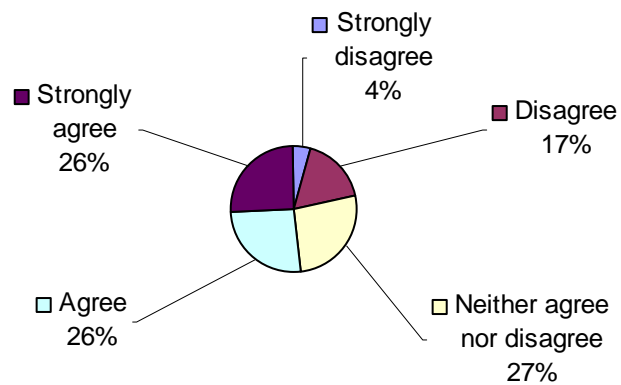


Figure 37. Question 4

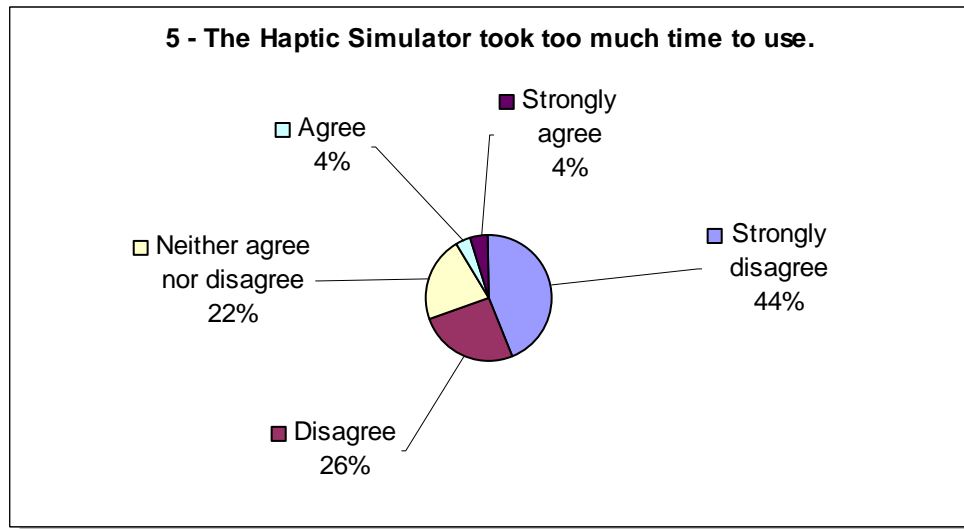


Figure 38. Question 5

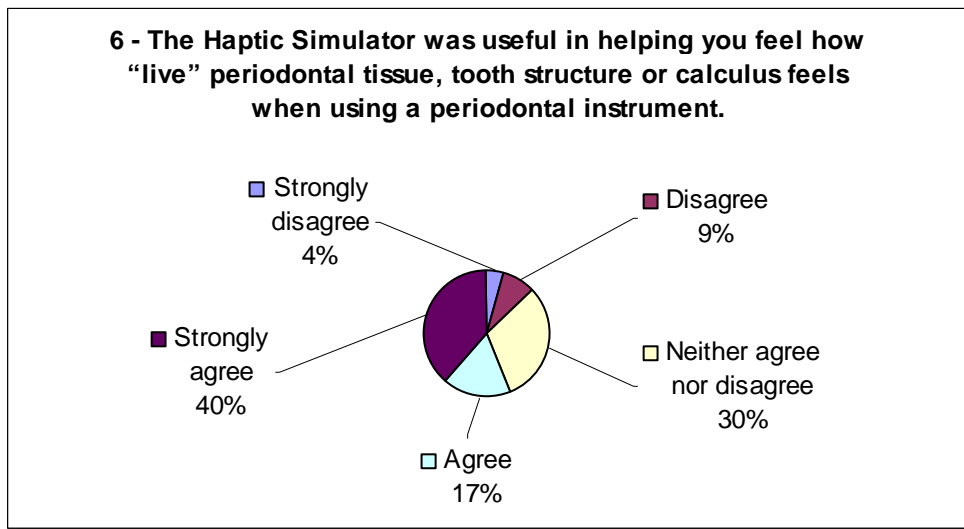


Figure 39. Question 6

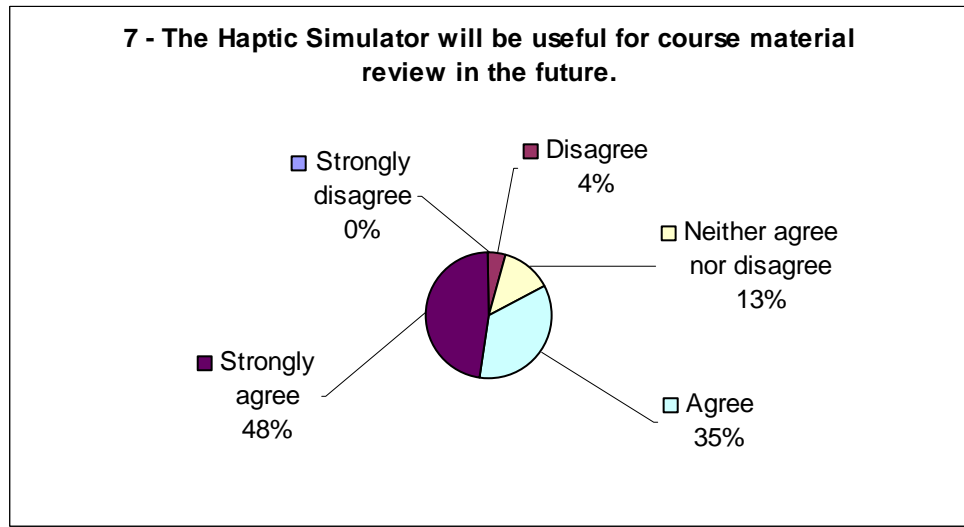


Figure 40. Question 7

5.3 Results of the preliminary evaluation

After the experiment, the Department of Periodontics at UIC reported the following conclusions:

- “The vast majority of users (21) adapted to the system very readily and found it easy to use and navigate.”
- “Only five of the responders used their computers for gaming purposes. However, this group adapted to the system faster than did non-gaming computer users.”
- “The vast majority (21) were fascinated by the technology and found it difficult to believe that they could feel the object shown on the monitor.”
- “Two of the users had a little difficulty with adaptation to the system. But even they were able to adapt and use it after several minutes of practice. Both rated the system lower than others.”

- “In the short time span allowed (10 minutes or less), all users were able to probe the onscreen gingival crevice area and establish its depth. They were able to feel the base of the pocket or crevice.”
- “We had difficulty with an oral anatomy instructor exceeding his time limit on the haptic device. He was so fascinated by the ability of feeling all of the tooth anatomy onscreen that he used the device for 15 minutes.”
- “Several users (10) applied too much pressure in using the haptic device stylus. This resulted in the onscreen probe becoming locked. Unlocking in such a situation is easily performed by pressing on a button on the stylus resetting the program. This reset procedure can be used to record excess pressure using the periodontal probe.”

The following are some of the comments given by the participants after the experiment:

- “A super experience! Congratulations on your progress.”
- “I like the ability to feel the movements seen on the screen monitor.”
- “I think this is a major breakthrough. The handpiece was easy to use and tactile sensitivity was excellent. It would make an excellent teaching system.”
- “If the finished product takes a lot of time to use and learn, students will not be receptive. After learning on a Dentech, it is hard to adapt to a computer. But looks very promising”.
- “A significant contribution to preclinical training in Periodontics.”

“The evaluation of the questionnaire suggests that the haptic-based periodontal simulator has great potential as a teaching instrument for learning periodontal probing.”

5.4 Validation of the simulator realism

A subsequent experiment was conducted by [Steinberg et al., 2006] at the Department of Periodontics at UIC to validate the realism of the periodontal simulator for training dental and hygiene students. “Twenty volunteer, experienced, male and female dental and hygiene faculty, from various dental clinical areas were used. Volunteers practiced before completing simulation exercise and rated it for realism (1 not realistic to 7 very realistic).”

“The analysis reported the following results with respect to the realism of the 3D images:

- Teeth: 6.60 ± 0.50
- Gingiva: 5.50 ± 1.50
- Explorer: 6.50 ± 0.69
- Periodontal probe: 6.24 ± 1.23

“Regarding the realism of the haptic feedback, the experiment reported the following results:

1. Teeth:

- Hardness: 6.25 ± 0.85
- Feel of surface: 6.00 ± 0.92
- Anatomy feel: 6.11 ± 0.74

2. Gingiva:

- Feeling: 3.50 ± 1.54

- Contrast to teeth: 4.90 ± 1.74
 - Anatomical feel: 4.20 ± 1.77
3. Instruments:
 - Explorer: 5.60 ± 1.19
 - Probe: 5.45 ± 1.36
 4. Instructions: 6.16 ± 1.49
 5. Teaching potential: 6.05 ± 1.32

The experiment demonstrated that the 3D images of the virtual mouth and instruments were considered highly realistic. In addition, haptic feedback was realistic for teeth and instruments whilst the gingiva was less so. Results reported by the experiment showed that the prototype haptics-based periodontal simulator was realistic enough to serve as a useful instruction tool with high teaching potential on periodontal procedures [Steinberg et al., 2006].

6 CONCLUSIONS

This thesis describes the research and development of a virtual reality dental simulator designed to facilitate the learning of diagnosis and treatment of periodontal diseases. To the best of our knowledge, this is the first haptics-based dental simulator designed exclusively for periodontics. Due to the importance of tactile feedback to perform periodontal procedures, haptics has demonstrated to be not only a helpful assistance in the learning process, but also a fundamental piece of the periodontal simulator to reproduce actual conditions encountered by a Dentist examining real patients. Periodontitis diagnosis and treatment as well as calculus detection cannot be successfully performed without a well-developed sense of touch. That skill cannot be taken for granted, and therefore, it needs to be learnt by dental and hygiene students. The haptics-based periodontal simulator is a small but first step towards that ultimate goal.

The efficient and novel integration between Coin and GHOST succeeded in a perfectly balanced computer load between a high-performance graphics and haptics rendering of relatively complex 3D geometry needed to produce a high level of real-time user interaction.

Finally, two experiments conducted by the Department of Periodontics at UIC using the simulator have validated its graphics and haptics realism as well as its potential in teaching Periodontal procedures.

6.1 **Future research and development**

This thesis offers a basic testbed for a broad spectrum of future development. An object-to-object collision detection could replace the point-based collision detection implemented by GHOST. This would allow a better simulation of the multiple contact

points between the dental instruments (like the scaler or the explorer) and the tooth surface. Of course, this would also require the use of a 6-DOF (input and output) force-feedback haptic device as the SensAble Premium 1.5 Phantom to provide resistance considering both the 3D position and orientation of the stylus. However, this is challenging because collision detection among multiple non-convex objects with highly complex geometry and penetration depth calculation are both computationally expensive.

In addition, in order to achieve a higher level of realism, graphics and haptics working volumes should not only match but also be collocated. In this way, the user would be able to “see” and “touch” at the same spot offering a useful tool to develop eye-hand coordination.

More exhaustive experiments of the periodontal simulator, with a larger sample of faculty and students from the Department of Periodontics, will be conducted in future to confirm or refute the results obtained by the preliminary validations.

Finally, this work can lead to the simulation of other dental procedures beyond Periodontics. Even medical procedures that require the simulation of tactile sensations could be developed based on the current implementation of the haptics-based periodontal simulator.

CITED LITERATURE

Autodesk: www.autodesk.com

Buchanan, J. A.: "Use of Simulation Technology in Dental Education," Journal of Dental Education; Vol. 65, No. 11, pp. 1225-30, 2001

Buchanan, J. A.: "Experience with Virtual Reality-Based Technology in Teaching Restorative Dental Procedures," Journal of Dental Education; Vol. 68, pp. 1258-65, 2004

Chan, D. C., Pruzler, K. B., Caughman, W. F.: "Simulation with Preclinical Operative Dentistry Courses, 3 year Retrospective Study," Journal of Dental Education (Abstract), Vol. 64, No. 3, pp. 190., 2000

Craig J.: Introduction to robotics, mechanics and control. Addison-Wesley, 1986

Digimation: www.digimation.com

Systems in Motion: www.coin3d.org/

Datta, V. K., Mandalia, M., Mackay, S. D., Darzi, A. W.: "Evaluation and Validation of a Virtual Reality Based Flexible Sigmoidoscopy Trainer," Gut, (Supplement) 48:A97-A98, 2001

Dean's Report, College of Dentistry: http://dentistry.uic.edu/news/dr/dr_09-04.pdf, September 2004

DenX: www.denx.com

Enexus, Inc.: www.enexus.com/gumdisease/

FLTK: www.fltk.org/

Hafernik, M. D.D.S.: www.austindental.com/more/gum.shtml

Immersion Medical: www.immersion.com/medical/

IOM: 1999 Institute of Medicine's report, To Err is Human, 1999

IDSS: grok.ecn.uiowa.edu/Projects/medsim.html

Jasinevicius T.R., Landers M., Nelson S., Urbankova A.: "An Evaluation of Two Dental Simulation Systems: Virtual Reality versus Contemporary Non-Computer-Assisted", Journal of Dental Education, Vol. 68, No. 11, pp. 1151-1162, 2004

KaVo: www.kavousa.com/products/dental_education/dse/dse.asp?navid=5200&lan=Us

Mehta, A. C., Ost, D., Salinas, S. G., Sanchez, D. E., DeRosiers, A., Tasto, J. L., Britt, E.: "Objective Assessment of Bronchoscopy Skills by a Bronchoscopy Training Simulator," American Journal of Respiratory and Critical Care Medicine; Vol. 161, No. 3, pp. A234, 2000

Montanari, L.: “Haptic rendering of a virtual tooth: state of the art, issues, solutions and techniques”, Master of Science in Computer Science thesis, UIC, 2003

Novint Technologies: www.novint.com/VRDTS.htm

Peterson D.: www.dentalgentlecare.com/scaling__root_planning.htm

Racine Dental Group: racinedentalgroup.com/services/services_periodontal.html, 2006

Reachin Core Technology: www.medica.de/cipp/md_medica/custom/pub/content,lang,2/ticket,g_a_s_t/oid,5984, 2006

Rowe, R., Cohen, R.: “Virtual reality bronchoscopy simulator”. Anesthesiology; (abstract) Vol. 93(3A), pp.1219, 2000

SensAble Technologies: www.sensable.com

Simulife Systems: amib.jouy.inra.fr/valo/simulife/simulife_en.htm, 2002

Spiller: www.doctorspiller.com/Gum_Disease.htm, http://www.doctorspiller.com/Treatment_of_Perio.htm

Steinberg, A. D., Banerjee, P., Drummond, J., Zefran, M.: “Progress in the Development of a Haptic/Virtual Reality Simulation Program for Scaling and Root Planning,” Journal of Dental Education, Vol. 67, No. 2, pp. 161, 2003

Steinberg, A., Drummond J.L., Bashook, P., Zefran M., and Ashrafi S., A haptic, 3D, Virtual Reality Dental Training Simulator Reality Validation, ADEA <http://iadr.confex.com/iadr/2006Orld/techprogram/abstract72559.htm>, 2006

StereoGraphics – Real D: www.reald.com/scientific/

Pham, T., Serafimovska, D., Elhajj: “Virtual Nursing Simulator with Haptic Force-Feedback for Oral Hygiene”, cse-reu.secs.oakland.edu/data/finalpptREU/thuy.ppt, 2006

Wong, T., Darzi, A., Foale, R., Schilling, R.J.: “Virtual reality permanent pacing: validation of a novel computerized permanent pacemaker implantation simulator.” J Am Coll Cardiol (Suppl) Vol. 37, pp. 493A-494A, 2001

VITA

NAME: Cristian Javier Luciano

EDUCATION: Bachelor of Science, Computer Science (Ingeniería en Sistemas de Información)
Universidad Tecnológica Nacional (UTN), Córdoba, Argentina, 1994

GRADUATE STUDIES: Master of Science, Computer Science
University of Illinois at Chicago (UIC), Illinois, 2006

Master of Science, Industrial Engineering
University of Illinois at Chicago (UIC), Illinois, 2000

RESEARCH EXPERIENCE: January 2002 - present:
Research Assistant
Industrial Virtual Reality Institute, UIC, IL

January 2001- January 2002
Staff
Electronic Visualization Laboratory

January 1999 – January 2001:
Research Assistant
Industrial Virtual Reality Institute, UIC, IL

TEACHING EXPERIENCE: January 1995 - December 1998:
Research and Teaching Assistant
University Center for Development of Automation and Robotics, UTN, Argentina

HONORS: Link Foundation Fellowship, 2003

Fulbright-YPF Fellowship, 2001-2003

Fulbright-CONICOR Fellowship, 1999-2000

Argentine Ministry of Culture and Education Fellowship, 1999-2000

CONICET Fellowship (National Scientific and Technological Research Council of Argentina), 1996-1998

PUBLICATIONS: Luciano, C., Banerjee, P. Lemole Jr., G.M. and Charbel, F.: “Second Generation Haptic Ventriculostomy Simulator Using The ImmersiveTouch™ System”, Proceedings Medicine Meets Virtual Reality, pp. 343-348, Long Beach, CA, 2006

Luciano, C., Banerjee, P., Florea, L., Dawe, G.: “Design of the ImmersiveTouch™: a High-Performance Haptic Augmented Virtual Reality System” CD ROM Proc. Of Human-Computer Interaction (HCI) International Conf., Las Vegas, NV, 2005

DeFanti, T., Banerjee, P., Luciano, C., Mehrotra, S.: “Realistic Cross-Platform Haptic Applications Using Freely-Available Libraries”, Proceedings of the 12th Symposium on Haptic Interfaces for Virtual Environment and Teleoperator Systems, Chicago, IL, 2004

Luciano, C., Banerjee, P., DeFanti, T., Mehrotra, S.: “A Framework For Efficient and More Realistic Haptics Applications”, Proceedings of 23rd ASME International Computers and Information Engineering Conference, Chicago, IL, 2003

Zhou, X., Luciano, C. , Banerjee, P. , Knight, J.: “Reconfigurable Driving Platforms in CAVE®”, SPIE, Virtual Reality and its Applications in Industry (VRAD), Bellingham, WA, 2002

Luciano, C., Banerjee, P., Mehrotra, S.: "3D Animation Of Telecollaborative Anthropomorphic Avatars", *Communications of the ACM*, vol. 44, no. 12, 2001, pp. 64-67., 2001

Luciano, C. and Banerjee, P.: 3D animation of telecollaborative anthropomorphous avatars using high-performance real-time inverse kinematics based on dual quaternions, IEEE Virtual Reality 2001, Yokohama, Japan, 2001.

Luciano, C. and Banerjee, P.: Avatar kinematics modeling for telecollaborative virtual environments, 2000 Winter Simulation Conference, Orlando, FL, 2000.

Luciano, C. and Banerjee, P.: Inverse kinematics of intelligent avatars for process and product design using dual quaternions, 3rd World Congress on Intelligent Manufacturing Processes & Systems, MIT, Cambridge, MA, 2000.

Luciano, C. and Apóstoli, R. S.: Virtual reality environment for real time simulation, control and monitoring of robotic manufacturing flexible systems, 8th International Conference on Advanced Robotics (ICAR'97), Monterey, CA, 1997.

Morán, O. D., Luciano, C., Rosales, A. and Apóstoli, R. S.: Real time control and supervision system of a tutorial flexible robotic manufacturing cell, 4th IFAC Symposium Low Cost Automation, Buenos Aires, Argentina, 1995.

Luciano, C., Morán, O. D. and Apóstoli, R. S.: Manufacturing simulation in a robotic flexible system, 4th IFAC Symposium Low Cost Automation, Buenos Aires, Argentina, 1995.